



**Medtech32 Australia**  
**Version 5.1.3/6.x.1/7.x.0**  
**Medicare Australia Online**  
**Vaccine Product Mapping Update**  
**(October 2009)**

**Release Notes**



These Release Notes contain important information for all Medtech32 users.  
Please ensure that they are circulated amongst all your staff.  
We suggest these should be filed safely for future reference.

---

## Table of Contents

For further information on this release, or any other queries regarding the Vaccine Product Mapping Update (Oct 2009), please contact the Medtech Helpdesk on 1800 148 165, or email [ausupport@Medtechglobal.com](mailto:ausupport@Medtechglobal.com).

<b>Pre-requisites</b> .....	<b>3</b>
<b>Introduction</b> .....	<b>4</b>
<b>Installation</b> .....	<b>5</b>
<b>Setup</b> .....	<b>7</b>
Vaccine Product Mapping .....	7
Inactive Test Vaccine .....	9

---

## Pre-requisites

Please review the following prerequisites and ensure they are met prior to installation:

### **IMPORTANT NOTE**

**This Update is intended for Medtech32 Version 5.1.3 (BUILD 1456 OR ABOVE) OR 6.x.1 (ANY BUILD) OR 7.x.0 (ANY BUILD) ONLY. If you ARE NOT on Medtech32 Version 5.1.3 OR 6.x.1 OR 7.x.0, please DO NOT continue.**

This can be checked by logging into Medtech32 and selecting *Help ▶ About Medtech32*.

- Ensure the person(s) who will be performing the upgrade have read through these notes.  
**IMPORTANT:** This document contains valuable information that, if not read, could seriously affect the upgrade process and/or possible down time of your network.
- Ensure you are ALWAYS logged onto Windows with administrative rights when performing ANY installation, update or maintenance tasks.
- Ensure you have a **COMPLETE** backup of ALL databases located in the MT32\Data directory.
- Ensure ALL users (including remote users) have **LOGGED OUT** of Medtech32 and ALL scheduled utilities, backup or maintenance tasks that require access to the databases have been **STOPPED**.
- Ensure the **LAST** Database you have logged in **LOCALLY** on the Medtech32 Server is the one you would like this update to run on.  
**NOTE:** If unsure, simply login to the CORRECT database from the Medtech32 Server, then log out and close Medtech32 before continuing.

## Introduction

With the recent introduction of the new vaccine **Panvax – Influenza Vaccine (H1N1)**, the corresponding Medicare ACIR Vaccine Code for this new vaccine need to be added to Medtech32 in order to enable mapping from within Medtech32 Setup (*Setup ▶ Recall/Screening ▶ Vaccine Product Mapping*). After running this update, sites will be able to register this new vaccine to ACIR via Medicare Australia Online.

The following is a summary of what will be changed by this Update:


- It will add the new Medicare ACIR vaccine Panvax (PANVAX) as defined by Medicare Australia under Vaccine Product Mapping.
- It will default the Medtech32 Vaccine Code (*MT32 Vaccine*) to 'TEST', and the Medtech32 Vaccine Product Code (*MT32 Code*) to 'TEST' under Vaccine Product Mapping for Panvax.
- All existing Vaccine Product Mapping WILL NOT be altered.
- It will update the Vaccine Type of the existing Medicare ACIR vaccines (if the vaccine type had been changed since the last update) as defined by Medicare Australia.

## Installation

The Vaccine Product Mapping Update (Oct 2009) must be run on the Medtech32 Server machine. The following procedures ONLY need to be run ONCE for EACH practice (or once per database if your practice has multiple databases).


**NOTE:** If you are uncertain which computer is the MedTech32 Server, please contact your IT technician or service provider who has performed the MedTech32 installation and/or upgrade.

1. Please visit our website at [www.medtechglobal.com](http://www.medtechglobal.com).
2. Select **Region: Australia** from the Region dropdown list on the top right corner of the screen.

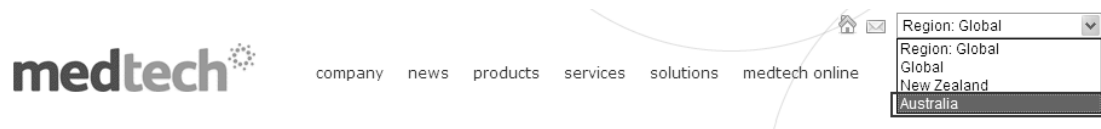

The Australia Home Page will be displayed.

3. Select from the Top Menu, **medtech online** ► **medtech32** ► **downloads**. The Australia Medtech32 Downloads page will be displayed.

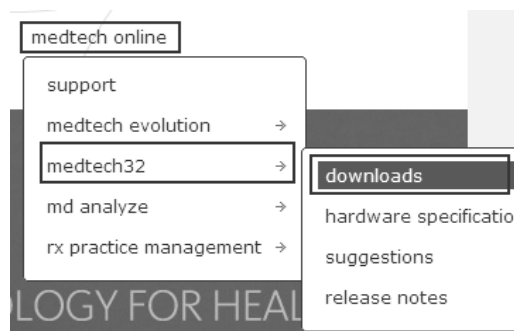


4. Here you will find the **Vaccine Product Mapping Update (Oct 2009)**.
5. If the File Download Security Warning dialogue box appears, select the **Run** option.
6. If the Open File Security Warning dialogue box appears, select the **Run** option.


7. The Update will then begin to run.



8. Click on the Button **Next** to begin running the Update.

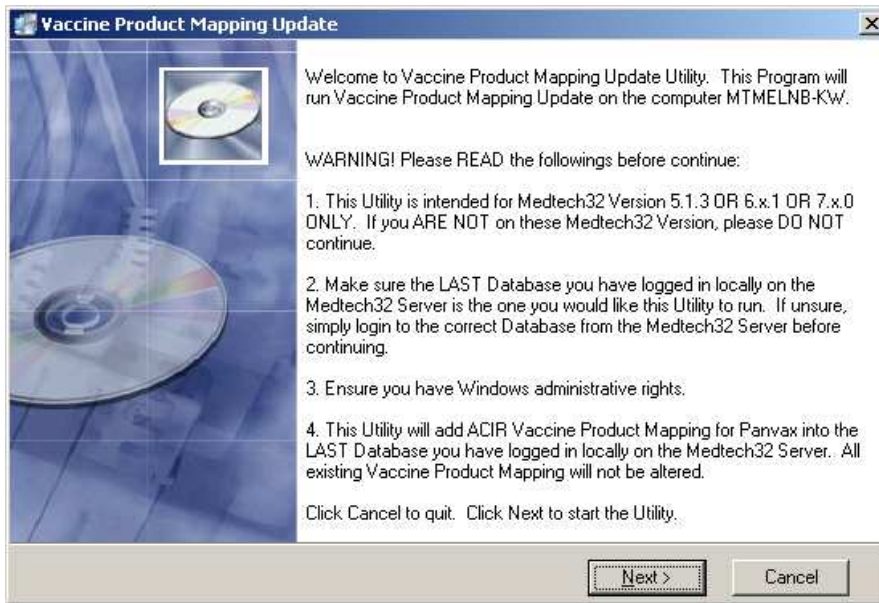

9. Once the Update is completed, the following screen will be displayed. Click on the Button **Finish** to exit the Update.

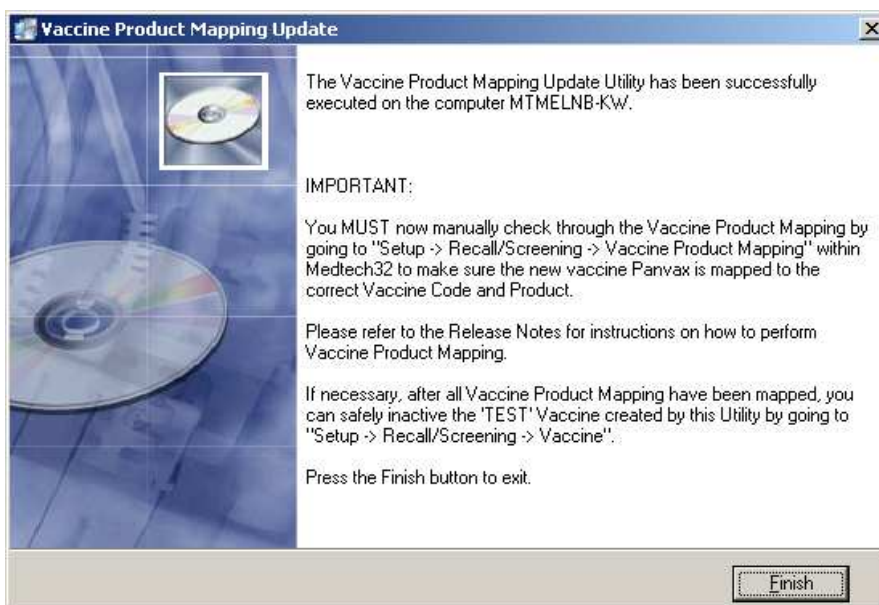

## Setup

### Vaccine Product Mapping


Setup ▶ Recall/Screening ▶ Vaccine Product Mapping

**IMPORTANT:** As Medicare Australia requires specific vaccine codes to be transmitted for ACIR Registration, **ALL** Vaccine Product Mapping must be mapped correctly.

Please follow the steps below to map current Vaccine Codes and Vaccine Product Codes in the Medtech32 database to the required Medicare Australia Vaccine Codes.

To map Vaccine Product Codes:

1. Select Setup ▶ Recall/Screening ▶ Vaccine Product Mapping. The Vaccine Product Code Mapping table will be displayed.

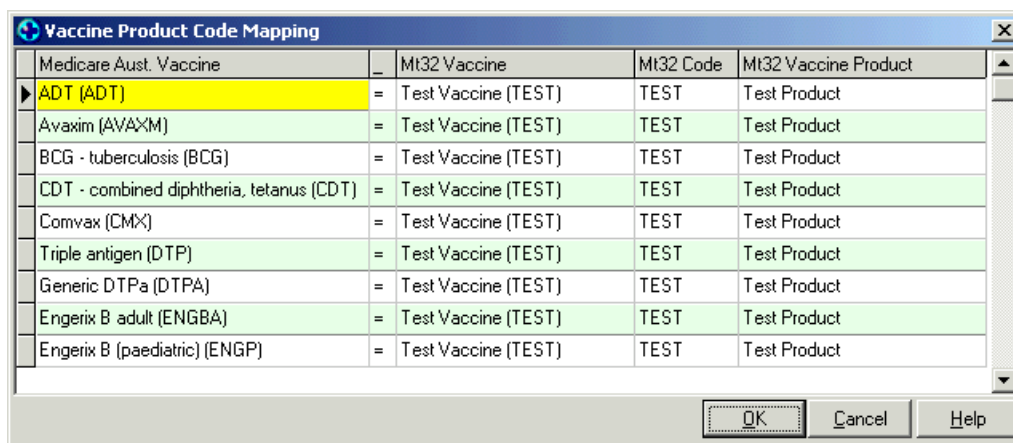

Medicare Aust. Vaccine		Mt32 Vaccine	Mt32 Code	Mt32 Vaccine Product
▶ ADT (ADT)	=	Test Vaccine (TEST)	TEST	Test Product
Avaxim (AVAXM)	=	Test Vaccine (TEST)	TEST	Test Product
BCG - tuberculosis (BCG)	=	Test Vaccine (TEST)	TEST	Test Product
CDT - combined diphtheria, tetanus (CDT)	=	Test Vaccine (TEST)	TEST	Test Product
Comvax (CMX)	=	Test Vaccine (TEST)	TEST	Test Product
Triple antigen (DTP)	=	Test Vaccine (TEST)	TEST	Test Product
Generic DTPa (DTPA)	=	Test Vaccine (TEST)	TEST	Test Product
Engerix B adult (ENGBA)	=	Test Vaccine (TEST)	TEST	Test Product
Engerix B (paediatric) (ENGP)	=	Test Vaccine (TEST)	TEST	Test Product


The left hand column Medicare Aust. Vaccine will show a list of all official Medicare ACIR Vaccines (description and code).

The middle column MT32 Vaccine will show a dropdown list of all Medtech32 Vaccines (description and code) that are currently setup in the Medtech32 database (Setup ▶ Recall/Screening ▶ Vaccine)


The next column MT32 Code will show a dropdown list of all associated Product Codes that are currently setup under the selected Medtech32 Vaccine (Setup ▶ Recall/Screening ▶ Vaccine – Product Tab)

The right hand column MT32 Vaccine Product will show the description of the Product Code that is selected under the column MT32 Code.


2. Select from the *MT32 Vaccine* dropdown list the Medtech32 Vaccine that matches the Medicare ACIR Vaccine.

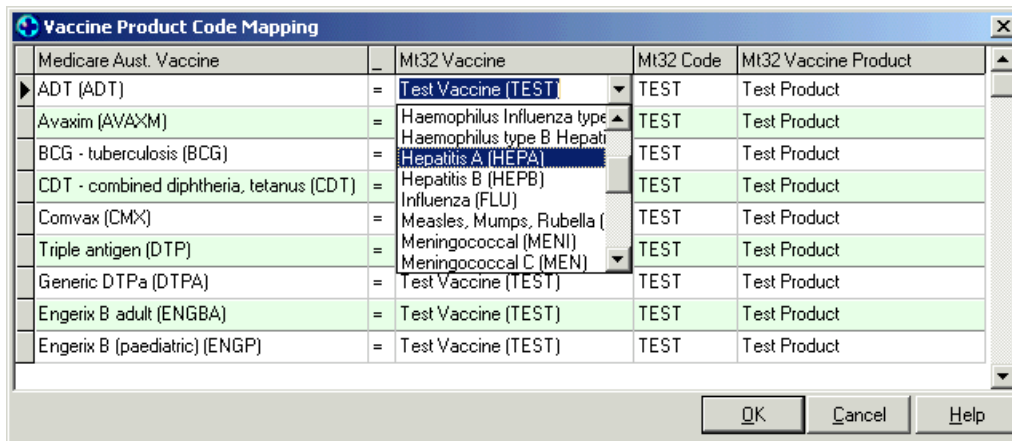

3. Select from the *MT32 Code* dropdown list the Medtech32 Product Code that matches the Medicare ACIR Vaccine.

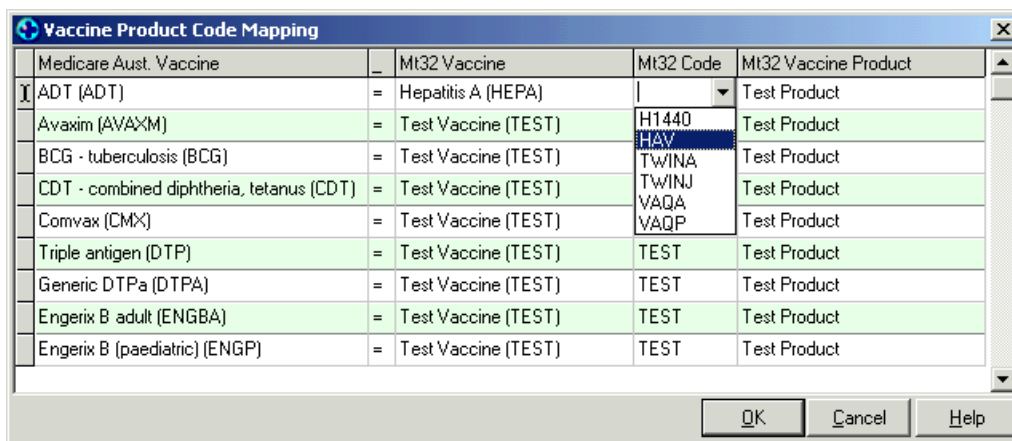

4. The *MT32 Vaccine Product* field will display the description of the Product Code that is selected under the column *MT32 Code*.

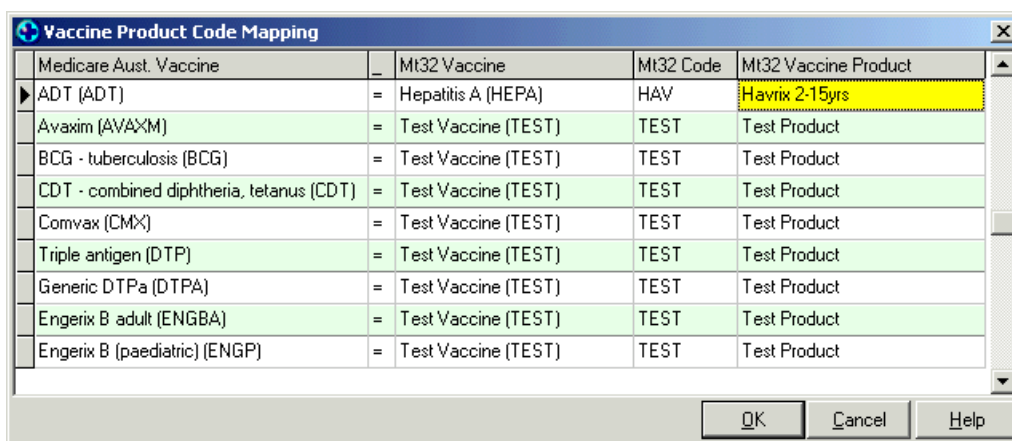

Once completed, the mapping will ensure that when sending an ACIR Registration to Medicare Australia from within Medtech32, the correct Medicare ACIR Vaccine Code will be transmitted.


**IMPORTANT:** If any Medtech32 Vaccine Codes (*MT32 Vaccine*) or Vaccine Product Codes (*MT32 Code*) have been made "inactive", the corresponding Medicare ACIR Vaccine Code (*Medicare Aust. Vaccine*) will **NO LONGER** be displayed for mapping.

Before inactivating any Medtech32 Vaccine Codes or Vaccine Product Codes, you **MUST FIRST** remap the corresponding Medicare ACIR Vaccine Code (*Medicare Aust. Vaccine*) to another **CURRENTLY ACTIVE** Medtech32 Vaccine Code or Vaccine Product Code.

## Inactive Test Vaccine

Setup ▶ Recall/Screening ▶ Vaccine

Once **ALL** Vaccine Product Mapping have been completed, you can safely inactive the 'Test Vaccine' created by the Utility by going to Setup ▶ Recall/Screening ▶ Vaccine.

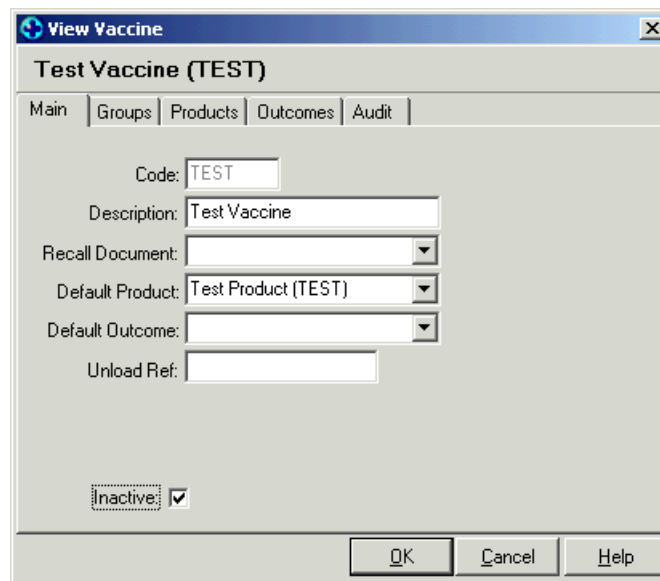

1. Open up the 'TEST' vaccine by double clicking on it.
2. Tick the Checkbox **Inactive**.
3. Click on the Button **OK**.

Should you require any assistance, please do not hesitate to contact the Medtech Helpdesk 1800 148 165, or email [ausupport@medtechglobal.com](mailto:ausupport@medtechglobal.com).